

Data Collection Statistics
Montezuma County - Colorado

Preliminary Validation

11/01/2010 - 11/30/2010

Parameter	Interval	Par Code	Data Recovery			Valid Data	
			No. Possible	No. Collected	% Collected	No. Valid	% Valid
Ozone	hourly	O3	720	706	98.1	704	97.8
Station Temperature	hourly	STP	720	720	100.0	720	100.0

Note: The percent valid is calculated against the number possible.


Automatic zeros and spans are performed daily on most ambient gas analyzers, therefore, no ambient data can be collected during this time. As a result, the maximum percent valid for ambient gas data typically can not be greater than 95.8.

Performance Goals:

Quarterly Criteria:
 100% of sites, >= 85% valid data capture
 90% of sites, >= 90% valid data capture
 80% of sites, >= 95% valid data capture


Monthly Criteria:
 100% of sites, >= 60% valid data capture
 90% of sites, >= 75% valid data capture
 80% of sites, >= 85% valid data capture

Montezuma County, Colorado - Cortez County Health Building

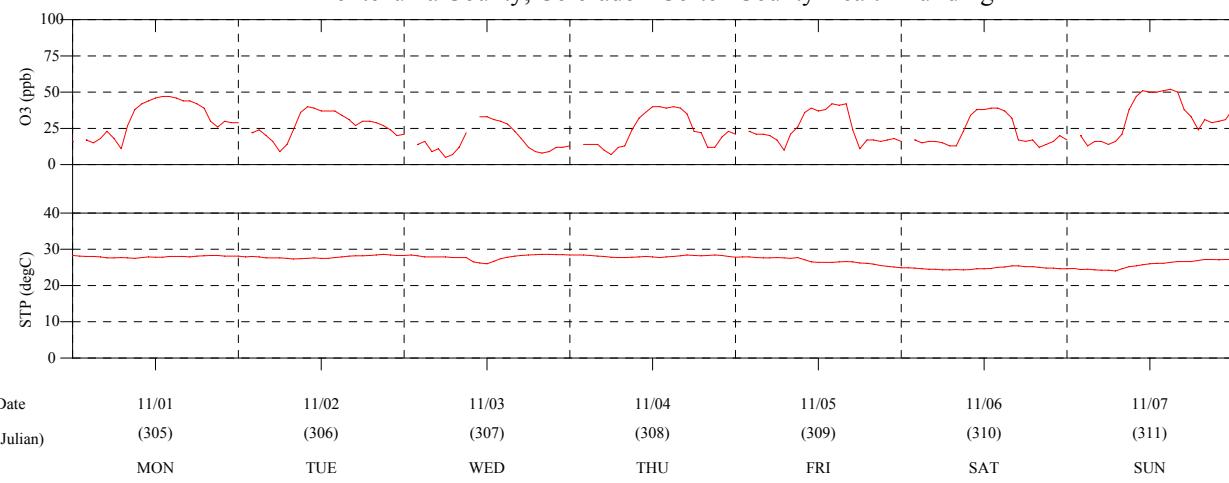

November 2010


Montezuma County, Colorado - Cortez County Health Building

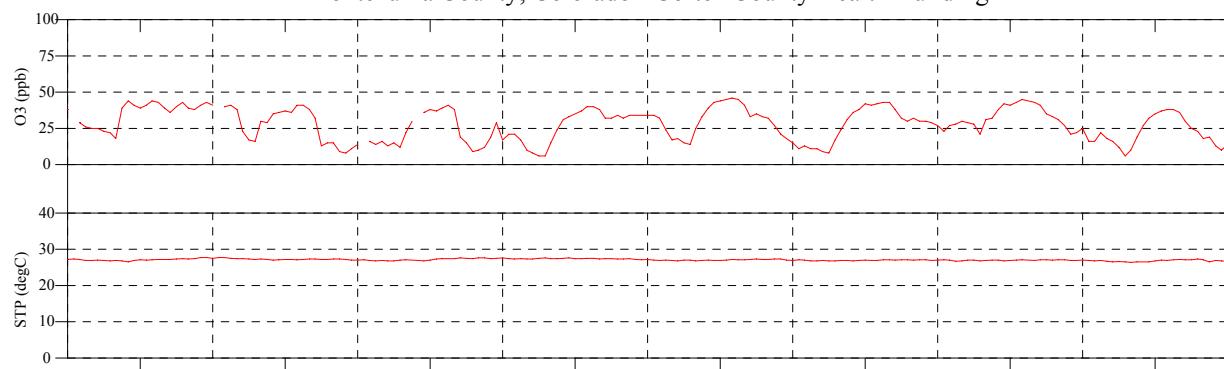

Date	11/08	11/09	11/10	11/11	11/12	11/13	11/14	11/15
(Julian)	(312)	(313)	(314)	(315)	(316)	(317)	(318)	(319)
	MON	TUE	WED	THU	FRI	SAT	SUN	MON


November 2010

Montezuma County, Colorado - Cortez County Health Building

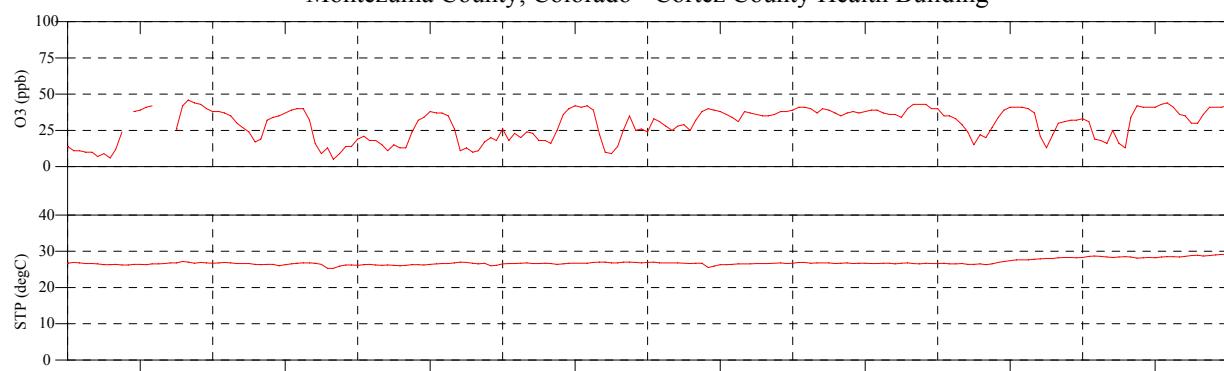

November 2010

Montezuma County, Colorado - Cortez County Health Building

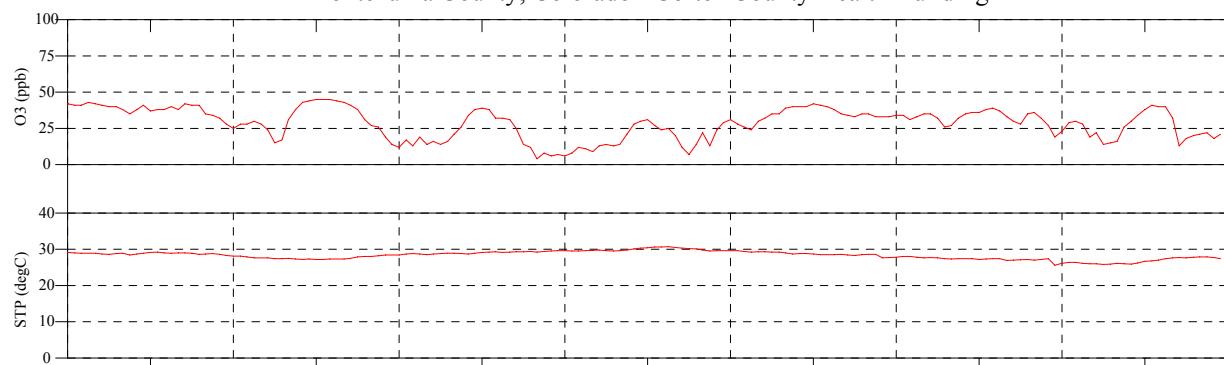

November 2010

Ozone
Summary of the Highest Daily Maximum 8-Hour Averages
Montezuma County - Colorado

Preliminary Validation
11/01/2010 - 11/30/2010

Date	Start and End Time of Daily Maximum 8-Hour Average	Daily Maximum 8-Hour Average (ppb)
11/07/2010	09 - 16	48
11/01/2010	10 - 17	45
11/25/2010	09 - 16	43
11/12/2010	09 - 16	42
11/14/2010	10 - 17	42
11/08/2010	09 - 16	41
11/23/2010	09 - 16	41
11/24/2010	00 - 07	41
11/13/2010	10 - 17	40
11/28/2010	08 - 15	40
0	Days this period with 8-hour averages > .075 ppm (75 ppb)	